BIOPLUX CLINICAL®

protocol quickguide

generic path
protocol

PLUX © 2010, all rights reserved

Channels setup

Choose the number of channels for monitoring and their names. When finished, press 'continue' to proceed to the next screen.

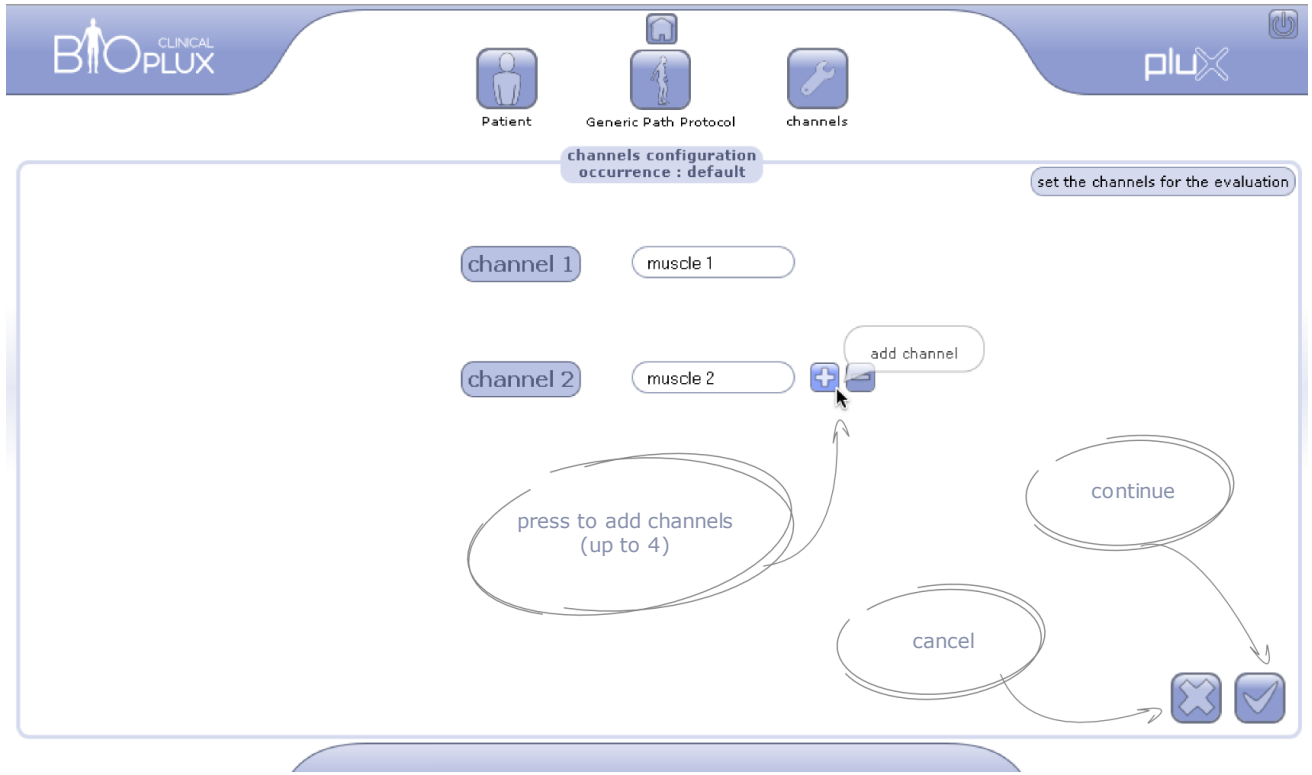

Calibration

Press 'start' to initiate the calibration, ensuring that the patient is at rest. Ask him to make the maximum contraction of the muscles. Stop the calibration. Press 'continue'.

Step 1

Here you can customize the path for the exercise. Clicking once with the left mouse button, appears a circle which means the first step. Then you can draw other circles that will determine the path, as forming a line. For deleting a cicle, you must click on it twice. You can also change the size of the circles, resulting in a shorter and more difficult path, simply using the bar of tolerance.

The path can be saved for future use. You only have to press the 'save' button and choose a name for it. For using an already created path, just click on a path on the list on the right.

When finish, press 'continue'.

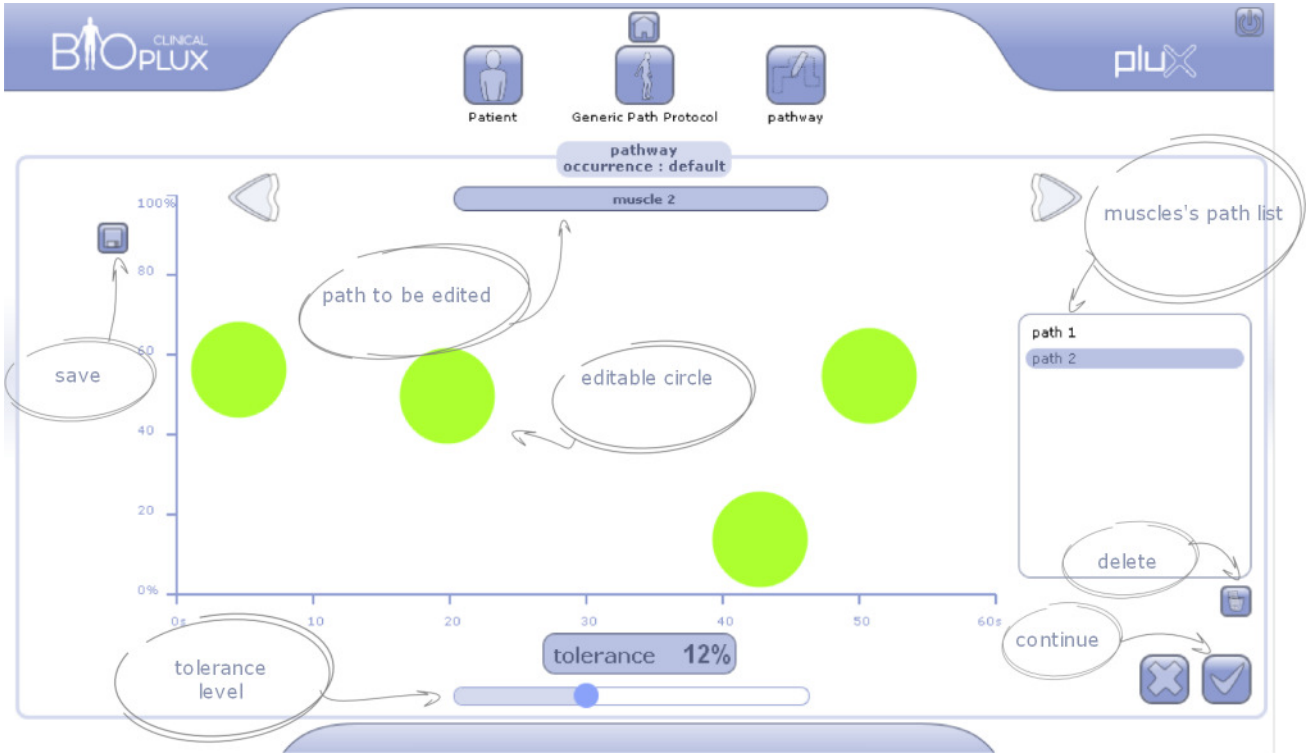

Save a path

Choose a name for the path and press 'confirm' to save it

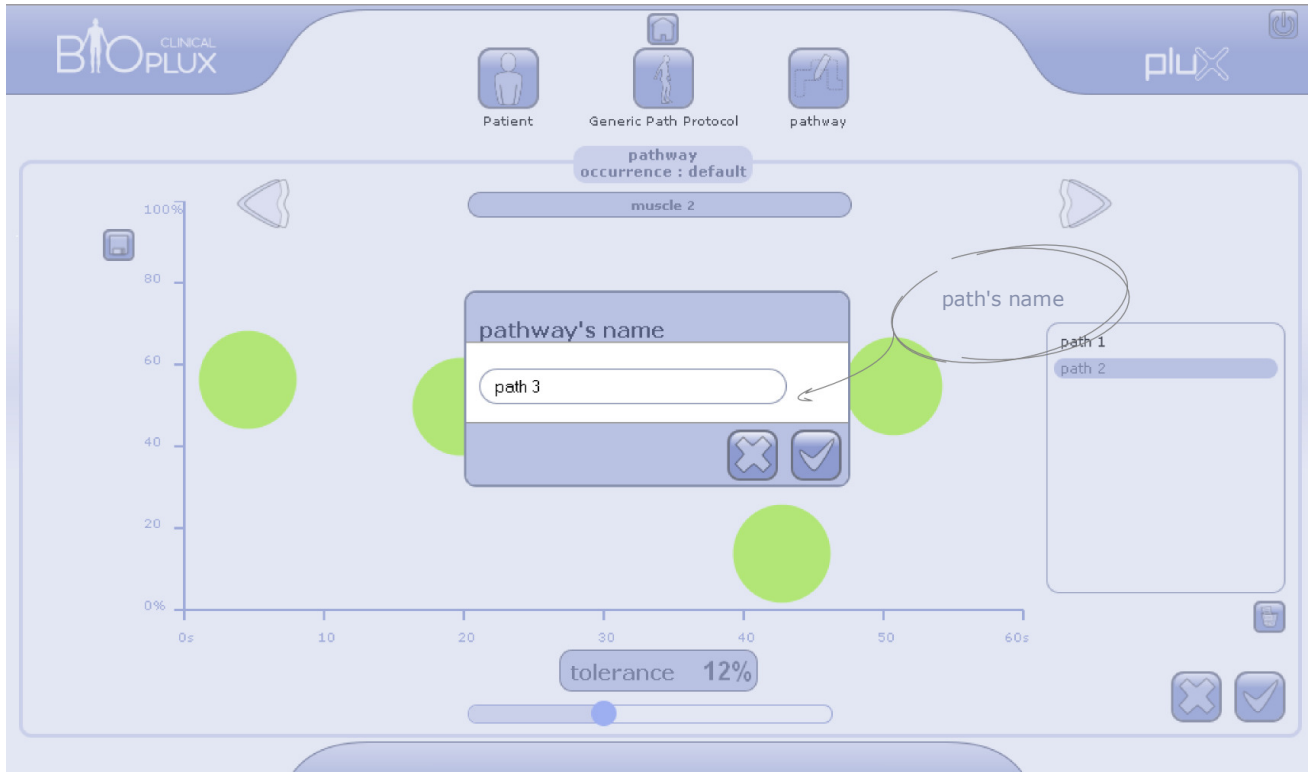

Step 2

In this exercise, the patient should try to keep going on a path. The longer he is on the path, more points the patient wins.

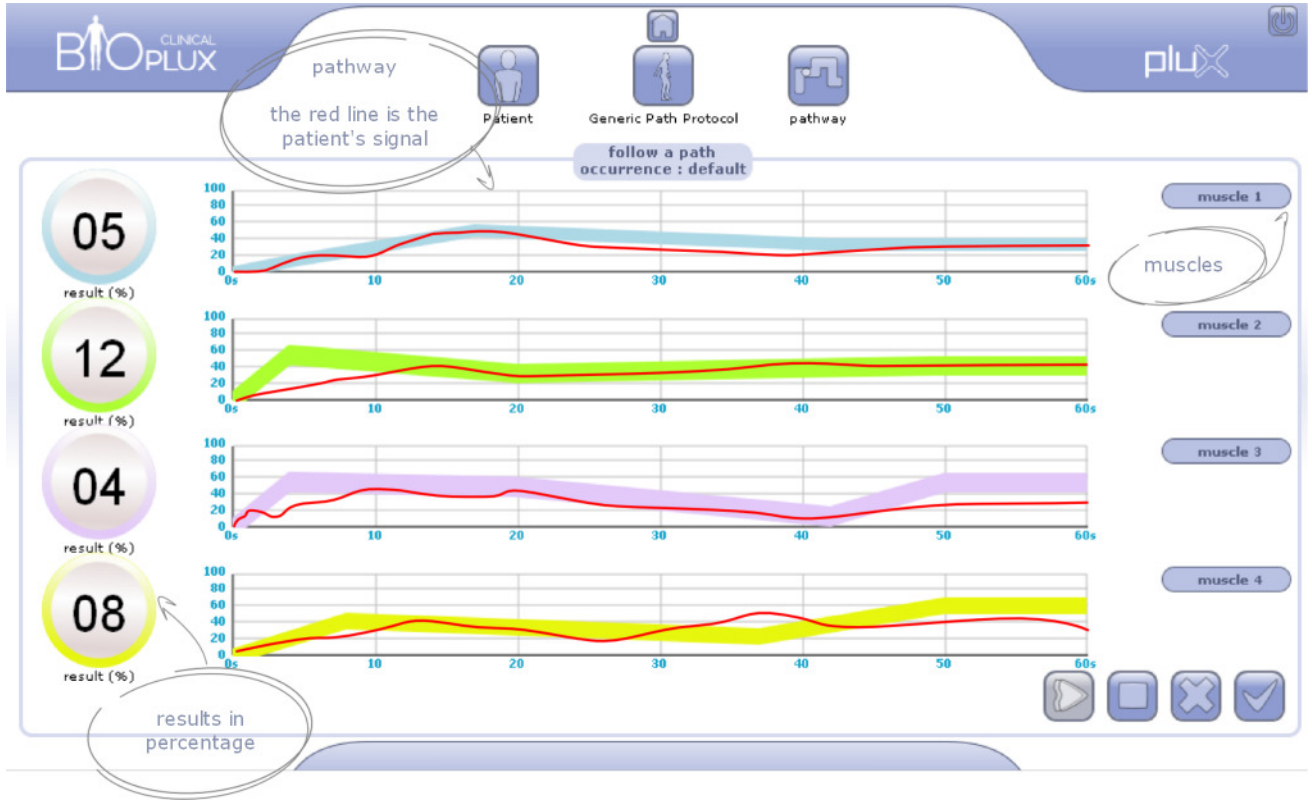

Report

Here you can view and print the report of the Protocol. In this screen you have access to patient information, protocol, and also all the results obtained.

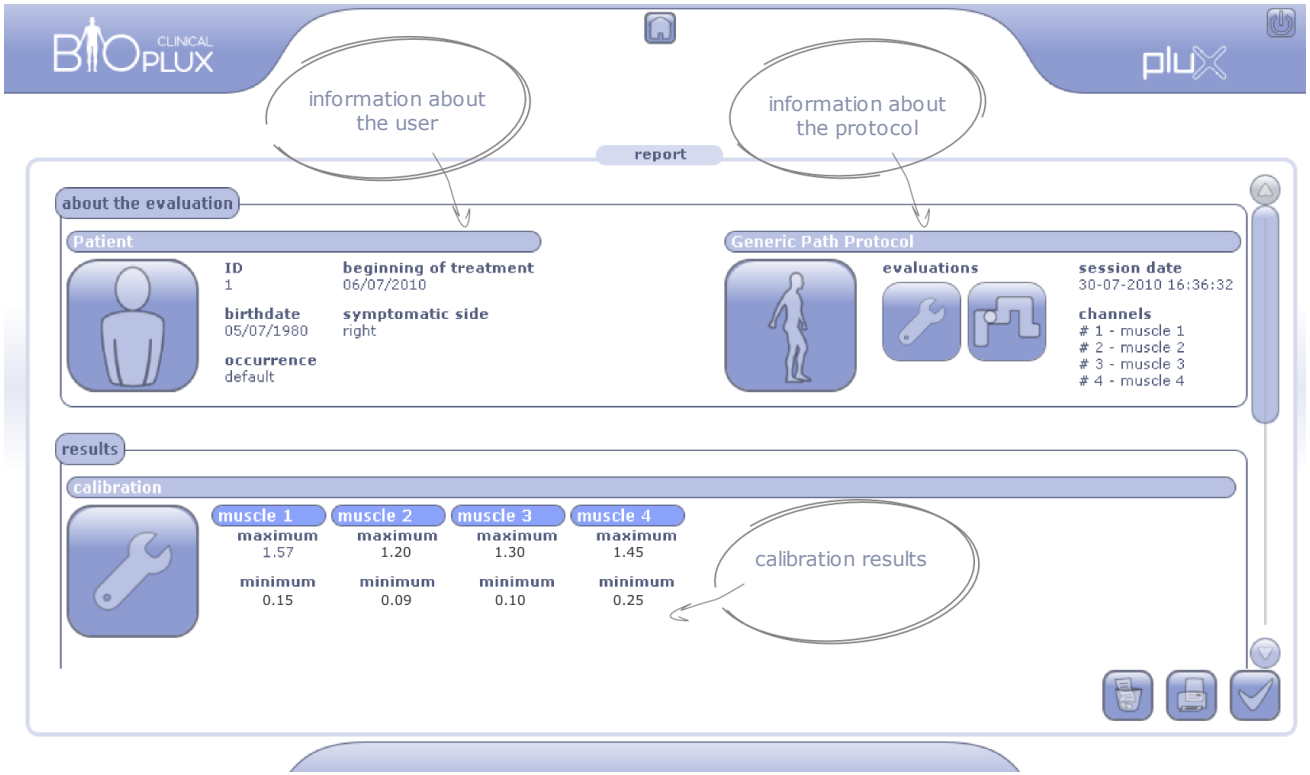

BIOPLUX CLINICAL
plux
total time (in seconds)
report
pathway
total time (s)
60
10
18
08
10
11.5
muscle 1 (tolerance 8 %)
muscle 2 (tolerance 12 %)
muscle 3 (tolerance 12 %)
muscle 4 (tolerance 10 %)
mean score
comments
maximum (in percentage) achieved
name of the technician
technician
space for comments
delete report
print report
conclude

www.bioplux.com

PLUX © 2010, all rights reserved